



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁵ : A61M 15/00	A1	(11) International Publication Number: WO 92/04069
		(43) International Publication Date: 19 March 1992 (19.03.92)

(21) International Application Number: PCT/SE91/00601

(22) International Filing Date: 10 September 1991 (10.09.91)

(30) Priority data:
9002895-2 12 September 1990 (12.09.90) SE(71) Applicant (for all designated States except US): AKTIEBO-
LAGET ASTRA [SE/SE]; S-151 85 Södertälje (SE).


(72) Inventors; and

(75) Inventors/Applicants (for US only): KÄLLSTRAND, Göran
[SE/SE]; Dragonvägen 1, S-237 00 Bjärred (SE). NILS-
SON, Per-Gunnar [SE/SE]; Bertrandsgratan 2A, S-212
14 Malmö (SE).(74) Agents: DANIELSSON, Sten et al.; AB Astra, Patent De-
partment, S-151 85 Södertälje (SE).(81) Designated States: AT, AT (European patent), AU, BB, BE
(European patent), BG, BR, CA, CH, CH (European
patent), CS, DE, DE (European patent), DK, DK (Euro-
pean patent), ES, ES (European patent), FI, FR (Euro-
pean patent), GB, GB (European patent), GR (Euro-
pean patent), HU, IT (European patent), JP, KP, KR,
LK, LU, LU (European patent), MC, MG, MW, NL,
NL (European patent), NO, PL, RO, SD, SE, SE (Euro-
pean patent), SU⁺, US.

Published

With international search report.

(54) Title: DISPOSABLE INHALER

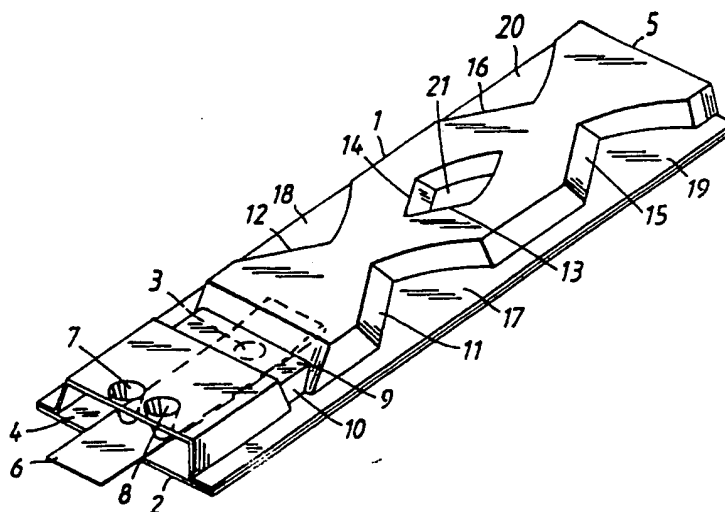

(57) Abstract

The invention relates to a disposable breath-actuated inhaler comprising a tubular housing forming an air flow path being open at both ends, one end forming an air inlet (4) and one end forming an air outlet (5), said housing comprising a compartment (3) for storing a pharmaceutical powder to be inhaled. The compartment (3) for storing the pharmaceutical powder is located close to the air inlet (4) and is covered by a thin foil (6) sealing the compartment in an airtight way which can be removed from the compartment from outside the housing, said housing being shaped with a constriction (9) adjacent the powder compartment (3) such that a turbulent air stream will be obtained at the constriction upon inhalation which will lift the powder out from the compartment (3) and mix the powder into the air stream.

+ DESIGNATIONS OF "SU"

Any designation of "SU" has effect in the Russian Federation. It is not yet known whether any such designation has effect in other States of the former Soviet Union.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	ES	Spain	MG	Madagascar
AU	Australia	FI	Finland	ML	Mali
BB	Barbados	FR	France	MN	Mongolia
BE	Belgium	GA	Gabon	MR	Mauritania
BF	Burkina Faso	GB	United Kingdom	MW	Malawi
BG	Bulgaria	GN	Guinea	NL	Netherlands
BJ	Benin	GR	Greece	NO	Norway
BR	Brazil	HU	Hungary	PL	Poland
CA	Canada	IT	Italy	RO	Romania
CF	Central African Republic	JP	Japan	SD	Sudan
CG	Congo	KP	Democratic People's Republic of Korea	SE	Sweden
CH	Switzerland	KR	Republic of Korea	SN	Senegal
CI	Côte d'Ivoire	LI	Liechtenstein	SU ⁺	Soviet Union
CM	Cameroon	LK	Sri Lanka	TD	Chad
CS	Czechoslovakia	LU	Luxembourg	TG	Togo
DE	Germany	MC	Monaco	US	United States of America
DK	Denmark				

Disposable inhaler.Technical field of the invention.

5

The present invention relates to a breath-actuated disposable inhaler of the kind having a generally tubular shape having two ends, one end forming an air inlet and one end forming an air outlet, the inhaler containing a pharmaceutical powder comprising particles of a respirable size which is to be inhaled.

10

Background of the invention.

15

Disposable, breath-actuated inhalers of the kind described above are for instance disclosed in WO 89/01348, US-A-4,265,236 and EP-A-0404454.

20 EP-A-0404454 discloses a disposable, breath-actuated inhaler comprising a chamber for a pharmaceutical powder, said chamber being provided with an air inlet and with an air outlet. The air inlet and outlet are covered by a common cover. The powder is disposed loosely in said
25 comparatively large chamber which means that the powder not necessarily will be located at that location at which the air flow is most efficient.

US-A-4,265,236 discloses a tubular disposable, breath-actuated inhaler comprising a flexible tube, the ends of which normally being sealingly inserted into each other.
This kind of seal will not necessarily be moisture-proof. There furthermore is a risk that some amount of the powder may fall out of the inhaler when the ends of the
35 tube are pulled apart.

WO 89/01348, in the embodiment most of interest here, discloses a tubular, disposable inhaler which is sealed in

both ends by means of twist-off caps. The pharmaceutical powder is loosely disposed in the inhaler and, as in the other inhalers described above, there is a risk that some powder is lost when the inhaler is opened.

5

The objects of the invention are to provide a disposable inhaler of the kind described above in which the dose of pharmaceutical powder can be determined accurately and in which the pharmaceutical powder can be stored hermetically sealed and moisture-proof. The dose delivered by different specimens of the same inhaler should generally be constant. The inhaler finally should be easy to prepare for use and easy to use as well as being easy and cheap to manufacture.

15

Brief description of the inventive concept.

The above objects are achieved in that the disposable inhaler is provided with the features set forth in the appended main claim. Advantageous embodiments are set forth in the dependent claims.

20

25 Brief description of the appended drawings.

Fig 1 shows a perspective view of an inhaler according to the invention,

Fig 2 shows a perspective view of an inhaler according to Fig 1 but showing the two main parts of the inhaler in an unassembled state,

30

Figs 3A - 3C show different stages in the opening of the powder compartment of the inhaler of Fig 1,

Fig 4 shows an end view of the air inlet of the inhaler in Fig 1,

35

Figs 5 - 7 show different possible embodiments of the constriction adjacent the powder compartment.

Detailed description of a preferred embodiment of the invention.

5 A preferred embodiment of the invention is disclosed in Figs 1 - 4. In Fig 1 the inhaler can be seen in a fully assembled condition and ready for use. As can be seen, the inhaler essentially comprises two elongate main parts, an upper part 1 which is made of a moulded sheet of
10 plastic material and a lower part 2 preferably made of aluminium foil laminated with plastic. The upper part 1 is U-shaped with a substantially rectangular shape. The width of the upper part is several times the height. The lower part is generally flat and the two parts thus form a
15 tubular housing defining an air conduit or air flow path with an air inlet 4 and an air outlet 5. A part-spherical depression or recess 3 indicated with a dashed line is located close to the air inlet 4. The recess 3 forms a powder compartment and is covered by a tape 6
20 which preferably is made of aluminium foil, also laminated with plastic.

As indicated, the end of the part of the tape 6 covering the recess 3 is located between the recess 3 and the air
25 inlet 4. The tape is attached to the lower part 2 around the powder compartment by means of a relatively weak weld 22 which can be seen in Fig 2. The end of the tape is attached by a comparatively large and thus stronger weld in front of the compartment, as seen in the intended
30 direction of the air flow. The free part of the tape 6 is bent backwards over the recess 3 and extends out through the air inlet 4. The free part of the tape is guided and held by two conical projections 7,8 extending downwards from the upper part 1.

35

A constriction in the flow path in the form of a ridge 9 oriented perpendicularly relative to the direction of the flow path is located above the powder compartment. The

ridge is formed as a depression 9 in the upper part 1. The ridge is delimited at each end by an abutment 10.

The inhaler is further provided with deaggregation means after the powder compartment, as seen in the direction of the intended air flow through the inhaler. These deaggregation means comprise a number of oblique planar surfaces which are oriented at an angle of about 30° relative to the longitudinal direction of the inhaler, it surprisingly having been found that the most efficient angle of a planar surface relative to the air flow direction for disintegrating powder agglomerations is about 30° . Since the air flow will be deflected to some extent by the planar surface, the flow direction will not coincide fully with the longitudinal direction, but the above angle has been chosen as being the best compromise. The planar surfaces are oriented generally perpendicularly relative to the lower part 2, or at least as perpendicularly as the method of manufacturing the inhaler allows. The planar surfaces are located in such a way that their projections onto a cross-sectional plane substantially cover the entire cross-section of the inhaler. The projections preferably should overlap to some extent in order to ensure that any larger particles or agglomerations entrained in the air flow will impact on at least one such surface. In the preferred embodiment the planar surfaces 11, 12, 13, 14, 15, 16 are located on the upstream ends of two pairs of indentations 17, 18; 19, 20, formed into the sides of the upper part 1 and on the upstream end of a central depression 21 located between said indentations forming an island in the flow path. The downstream ends of said indentations and said depression taper in the direction of the air flow and have a smooth, rounded shape in order to obtain good aerodynamic conditions without any areas where the powder entrained in the air flow could settle.

The two main parts of the inhaler are shown separated in Fig 2. Apart from the details shown in Fig 1, the powder compartment 3 is shown opened, the tape 6 having been pulled outwardly through the air inlet. The shape of the (broken) weld 22 can be seen on the tape 6 and around the powder compartment 3. As can be seen, the shape of the weld has been chosen to be the perimeter of a square oriented with one diagonal parallel with the longitudinal extent of the inhaler. This means that the disengagement of the tape from the lower part 2 will be facilitated since the tearing action will both start and end at a corner. Since the weld holding the inner end of the tape is broad and strong, the user will feel when the compartment has been uncovered by means of the increased resistance.

Figs 3A - 3C show different stages in the opening of the powder compartment 3 by pulling the tape 6, thus exposing the powder 23.

The end view in shown in Fig 4 more clearly illustrates the inter-relationship between the upper part 1, the lower part 2, the powder compartment 3, the tape 6, the conical projections 7, 8, the ridge 9 and the abutments 10.

When the inhaler is to be used, the inhaler is held more or less horizontal with the flat half 2 facing downwards. The free end of the tape 6 is pulled outwardly and the powder in the powder compartment 3 is exposed. The two conical projections 7, 8 will hold the tape 6 flat against the lower part 2 and thus prevent the tape from occluding the constriction in front of the powder compartment. The user then inserts the air outlet into the mouth and inhales through the inhaler. The resultant air flow through the inhaler will become very turbulent in the region of the constriction and the pharmaceutical powder will be lifted out of the powder compartment and mixed with the air flow. Any particles adhering to the tape may

also be entrained with the air flow since the part of the tape originally covering the powder compartment also will lie directly in the flow path.

- 5 Tests have shown that the dose leaving a typical powder compartment (about 0.5 mg) located at a constriction having an area of about 10 - 12 mm² will remain essentially constant at air flow rates varying from 30 l/min to 60 l/min.

10

- The powder-laden air will then flow from the constriction to the deaggregation means. The angle of attack of the oblique surfaces will entail that the lighter particles, i. e. the particles within the respirable range, < 6µm, will be deflected from the surface without sticking thereto and thus mainly will follow the air flow, whereas the heavier particles and agglomerates will impact on and rebound from the planar surfaces and in this way be broken up into smaller particles. As mentioned above, an angle of about 30° may be optimal.

20

- In this case tests again have shown that the percentage of particles within the respirable range in the dose to be inhaled will remain substantially constant at air flow rates ranging from 30 l/min to 60 l/min.

25

- That the dose of respirable particles remains substantially constant over a wide range of air flows is important in order to minimize the difference between patients with different inhalation capacities.

30

- It should be noted that the tubular shape of the inhaler makes it possible to mount a rubber ball or similar over the air inlet. By the means thereof the powder could be ejected from the inhaler into the throat of the patient in synchronization with the breathing of the patient by a helper if the patient should be incapable to use the inhaler by himself.

35

As mentioned above, the lower part 2 of the inhaler as well as the tape 6 preferably are made of aluminium foil laminated or coated with a suitable plastic. The aluminium
5 will ensure the desired protection against moisture whereas the plastic will ensure that the tape can be welded to the lower part and that the lower part can be welded to the upper part. The lower part may for instance consist of a aluminium foil having a thickness of 45 μ
10 which on one side is covered with a layer of oriented polyamide which is 25 μ thick and on the other side is covered by a layer of polypropene which is 60 μ thick. The upper part is preferably made of polypropene being 300 or 400 μ thick. The upper part can be transparent so
15 that the user can see if the dose has been ejected from the powder compartment.

The tape may be made of a laminate having a "peel"-effect comprising polyester, aluminium and a layer comprising a
20 polymer mixture of polybuten and polypropene.

The choice of material in the inhaler should be adapted to the drug to be used. The above materials have been chosen with a specific drug (budesonide) in mind, these materials
25 releasing a dose of this drug more easily.

The composition of the pharmaceutical powder of course is quite optional and the powder may for instance comprise a pure active substance, a mixture of different active
30 substances or a mixture of active substance(s) with adjuvant(s). It should be pointed out that the scope of choice of drugs is widened considerably due to the moisture-proof containment of the drug in the powder compartment.

35

The inhaler may be manufactured in the following way. A series of half-spherical indentations are formed in a strip of laminated aluminium foil in order to shape

powder compartments. The indentations are filled with drugs and are topped off by means of scrapers, which will ensure a substantially uniform size of the different doses. An aluminium tape laminated with plastic is then
5 welded over each indentation.

The lower parts are then welded to upper parts and the strip is cut to form individual inhalers which are ready for packaging and use. The upper parts are moulded from
10 sheets of plastic. In the moulding procedure care should be taken to ensure that the side walls of the upper part are as perpendicular as possible relative to the upper side in order to ensure an air flow which is as uniform as possible throughout the entire cross-section of the
15 inhaler. The function of the abutments 10 primarily are to prevent that the ridge forming the constriction is distorted during the welding process.

Possible modifications of the invention.

20 The invention of course can be modified in many ways within the scope of the appended claims.

Thus the ridge 9 forming the constriction can be designed
25 in different ways in order to enhance the lifting action of the air flow on the powder. Some examples thereof can be found in Figs 5 - 7.

Fig 5 illustrates how the ridge 9 can be provided with a
30 small hole 24 centrally above the powder compartment 3. When the patient inhales through the inhaler, additional air will be directed more or less perpendicularly down into the powder compartment, thus enhancing the turbulent action in the vicinity of the powder compartment.

35 Figs 6 and 7 illustrate two alternative embodiments wherein the ridge has been provided with an edge 25 resp 26 oriented along the longitudinal extent of the ridge and

which also will direct some air flow more directly into the powder compartment.

5 These embodiments will however require a higher degree of precision in the manufacturing in order to obtain the desired effect than the embodiment described above and will therefore be more difficult to manufacture.

10 The ridge 9 forming the constriction has been illustrated as being generally trapezoid in cross-section and as being generally rectilinear in longitudinal section. It should however be pointed out that the constriction may be shaped in many different ways within the scope of the appended claims.

15 The powder compartment can of course have another shape than a half-spherical shape and may for instance be elliptical, the minor axis thereof being parallel with the direction of the air flow, or may be otherwise trough-shaped. It is of course also possible to have several
20 indentations, for instance if it is desired to increase the dose in an exactly defined way.

25 The projections 7,8 can be shaped otherwise than conically and may for instance be shaped such that they direct a greater part of the air flow more directly past the powder compartment. They also could be integrated with the abutments 10.

30 The deaggregation means can be designed in other ways than in the form of planar surfaces oriented at an angle of about 30° relative to the direction of the air flow. This angle can be varied and the surface itself does not necessarily have to be planar.

35 The material in the lower part and the tape does not necessarily have to comprise aluminium and may be any

plastic material having the necessary impermeability and stiffness or having been treated to have these properties.

5 It is also conceivable to make the inhaler from a single sheet which is rolled or folded after having been moulded in an appropriate way.

CLAIMS.

1. Disposable breath-actuated inhaler comprising a
5 tubular housing forming an air flow path being open at
both ends, one end forming an air inlet (4) and one end
forming an air outlet (5), said housing comprising a
compartment (3) for storing a pharmaceutical powder to be
inhaled, c h a r a c t e r i z e d in that the
10 compartment (3) for storing the pharmaceutical powder is
located close to the air inlet (4) and is covered by a
thin foil (6) sealing the compartment in an airtight way
which can be removed from the compartment from outside the
housing, said housing being shaped with a constriction (9)
15 adjacent the powder compartment (3) such that a turbulent
air stream will be obtained at the constriction upon
inhalation which will lift the powder out from the
compartment (3) and mix the powder into the air stream.
- 20 2. Inhaler according to claim 1, c h a r a c t e r i z e d
in that said housing is formed of two main parts, one
moulded upper half (1) and one generally flat lower half
(2) having an indentation (3) forming the powder
compartment, said two halves (1, 2) being joined together
25 along their longitudinal sides.
3. Inhaler according to claim 1 or 2,
c h a r a c t e r i z e d in that the upper part (1) is
moulded from a thin sheet, preferably of plastics
30 material.
4. Inhaler according to claim 3,
c h a r a c t e r i z e d in that said constriction (9)
is formed as a depression in the upper side of said upper
35 part (1) which is oriented transversely relative to the
longitudinal extent of the tubular housing and located
above the powder compartment (3) formed in the lower half
(2) of the housing.

5. Inhaler according to any one of the preceding claims, characterized in that the lower half (2) is made of aluminium foil laminated with plastic.

5

6. Inhaler according to any one of the preceding claims, characterized in that the thin foil is in the shape of a tape (6) having one free end extending out through the air inlet (4), said tape being attached around the edges of the powder compartment (3) by means of relatively weak welds (22).

10

7. Inhaler according to claim 6, characterized in that the inner end of the tape (6) is attached to the lower half (4) between the air inlet (4) and the powder compartment (3), the tape (6) extending past, and being attached around, the powder compartment (3), the tape then being bent backwards about so as to extend out through the air inlet (4).

20

8. Inhaler according to claim 7, characterized in that the weak welds (22) form a point facing downstream in order to facilitate the initiation of the tearing action along the welds (22) when the tape (6) is to be pulled out through the air inlet (4) in order to expose the powder.

25

9. Inhaler according to any one of claims 6 - 8, characterized in that projections (7, 8) extend downwards from the upper half (1) between the powder compartment (3) and the air inlet (4) for holding the tape (6) against the lower half (2) of the housing in order to prevent the tape (6) from obstructing the air flow path.



35

10. Inhaler according to any one of the preceding claims, characterized in that deaggregation means

(11, 12, 13, 14, 15, 16) are located in the air flow path between the powder compartment (3) and the air outlet (5).

11. Inhaler according to claim 10,
- 5 c h a r a c t e r i z e d in that said deaggregation means comprise planar surfaces (11, 12, 13, 14, 15, 16) oriented about 30° relative to the longitudinal direction of the tubular housing, said surfaces being disposed generally perpendicularly to a plane through the
- 10 longitudinal axis of the tubular housing, a projection of the planar surfaces onto a cross-section of the housing substantially covering said cross-section.

1/3

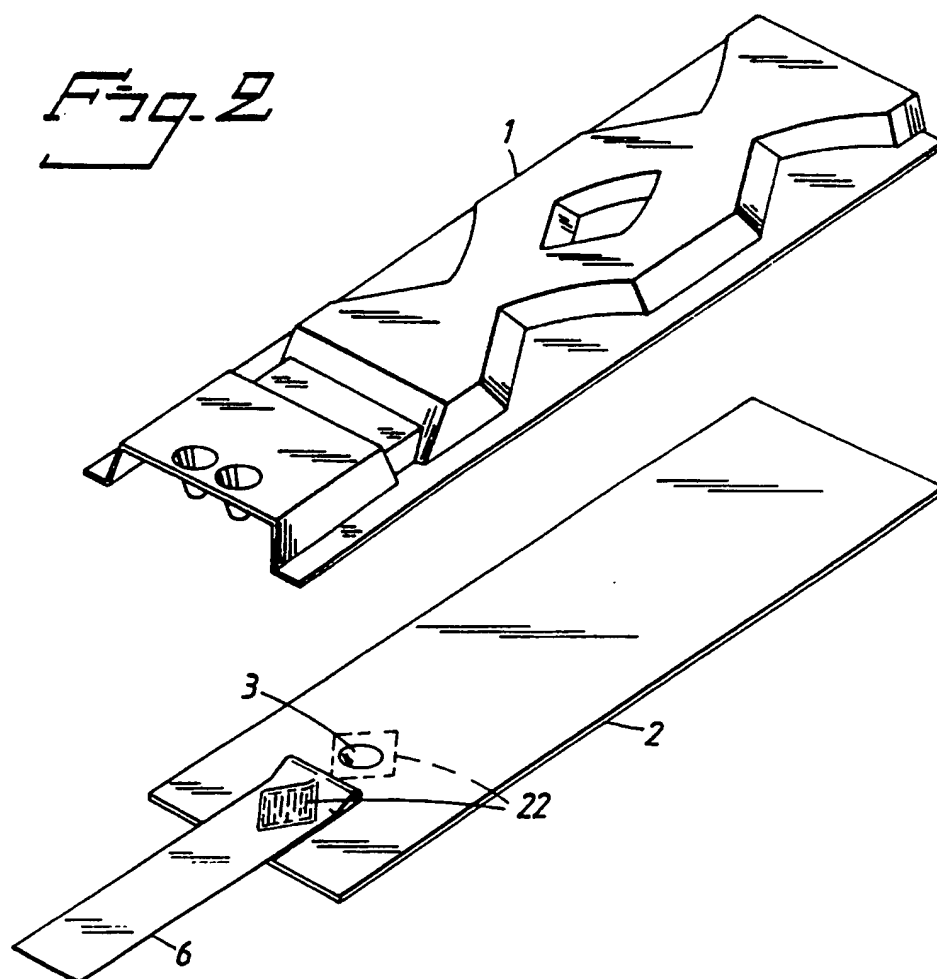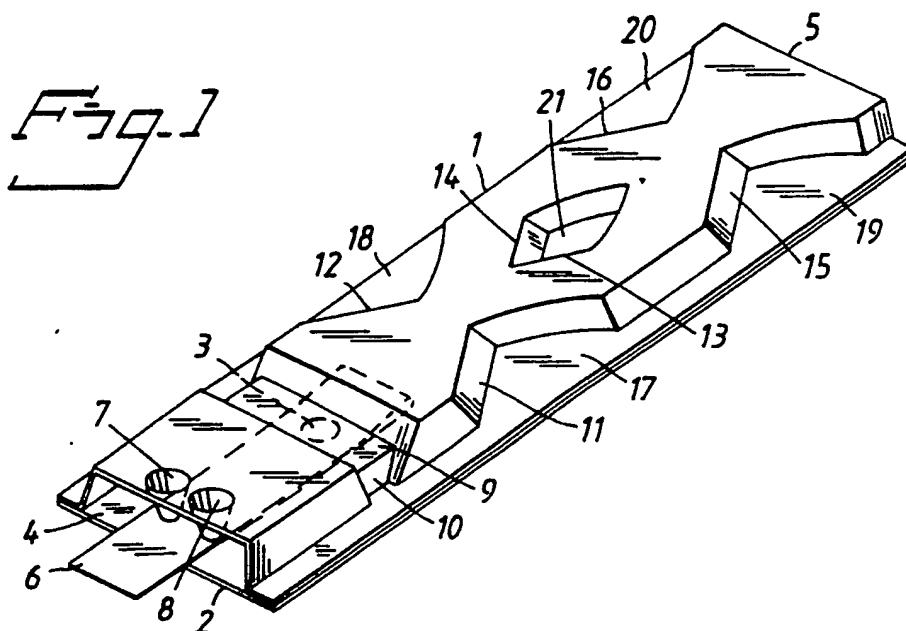

SUBSTITUTE SHEET

2/3

Fig. 3A

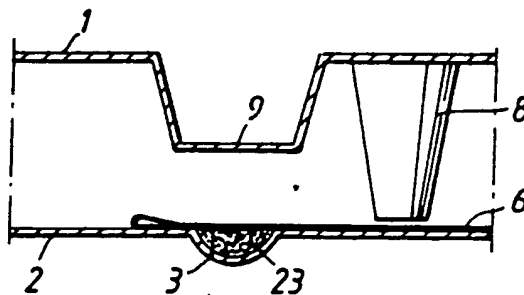


Fig. 3B

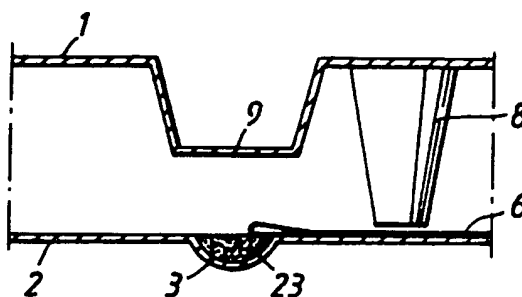


Fig. 3C


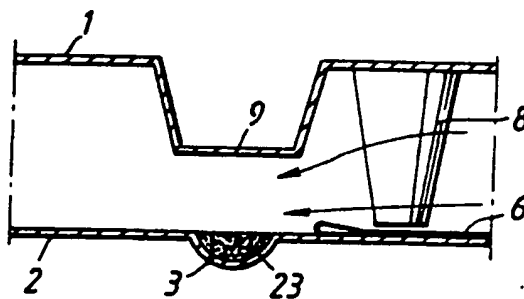


Fig. 4

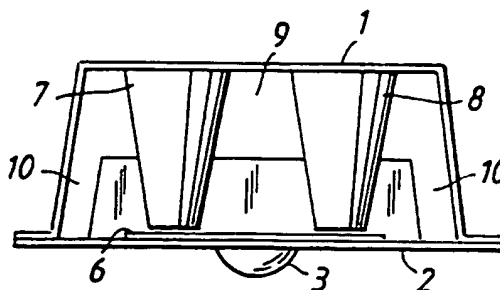

3/3

Fig. 5

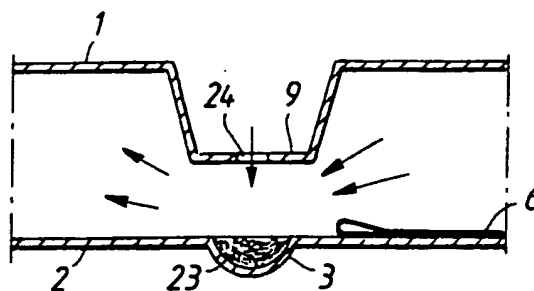


Fig. 6





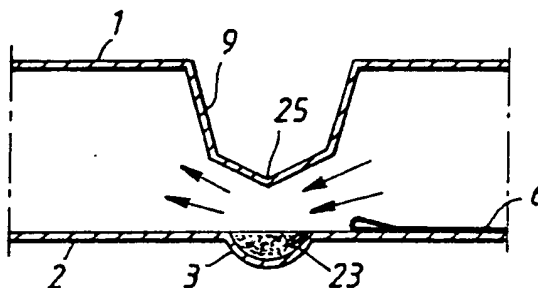


Fig. 7

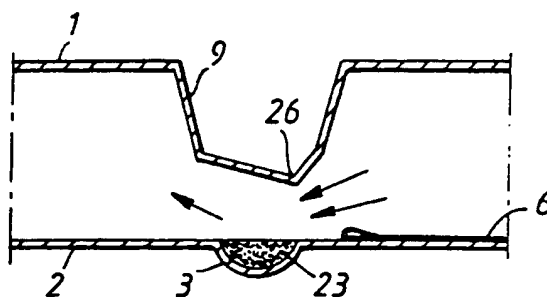

INTERNATIONAL SEARCH REPORT

International Application No PCT/SE 91/00601

I. CLASSIFICATION OF SUBJECT MATTER (If several classification symbols apply, indicate all) ⁶ According to International Patent Classification (IPC) or to both National Classification and IPC IPC5: A 61 M 15/00														
II. FIELDS SEARCHED <div style="text-align: center; border: 1px solid black; padding: 2px;">Minimum Documentation Searched⁷</div> <table style="width: 100%; border-collapse: collapse;"> <tr> <th style="width: 25%; border: 1px solid black; padding: 2px;">Classification System</th> <th style="border: 1px solid black; padding: 2px;">Classification Symbols</th> </tr> <tr> <td style="border: 1px solid black; padding: 5px; vertical-align: top;">IPC5</td> <td style="border: 1px solid black; padding: 5px; vertical-align: top;">A 61 M</td> </tr> </table>			Classification System	Classification Symbols	IPC5	A 61 M								
Classification System	Classification Symbols													
IPC5	A 61 M													
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in Fields Searched ⁸ SE,DK,FI,NO classes as above														
III. DOCUMENTS CONSIDERED TO BE RELEVANT⁹ <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 10%; padding: 2px;">Category *</th> <th style="width: 60%; padding: 2px;">Citation of Document,¹¹ with indication, where appropriate, of the relevant passages¹²</th> <th style="width: 30%; padding: 2px;">Relevant to Claim No.¹³</th> </tr> </thead> <tbody> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">EP, A1, 00404454 (FISONS PLC) 27 December 1990, see column 4, line 16 - line 46; figure 3 <div style="text-align: center;">--</div></td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">US, A, 4265236 (PACELLA) 5 May 1981, see abstract; figure 2 <div style="text-align: center;">--</div></td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">WO, A1, 8901348 (TEIJIN LIMITED) 23 February 1989, see abstract; figures 5-8 <div style="text-align: center;">-- -----</div></td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> </tbody> </table>			Category *	Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²	Relevant to Claim No. ¹³	A	EP, A1, 00404454 (FISONS PLC) 27 December 1990, see column 4, line 16 - line 46; figure 3 <div style="text-align: center;">--</div>	1	A	US, A, 4265236 (PACELLA) 5 May 1981, see abstract; figure 2 <div style="text-align: center;">--</div>	1	A	WO, A1, 8901348 (TEIJIN LIMITED) 23 February 1989, see abstract; figures 5-8 <div style="text-align: center;">-- -----</div>	1
Category *	Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²	Relevant to Claim No. ¹³												
A	EP, A1, 00404454 (FISONS PLC) 27 December 1990, see column 4, line 16 - line 46; figure 3 <div style="text-align: center;">--</div>	1												
A	US, A, 4265236 (PACELLA) 5 May 1981, see abstract; figure 2 <div style="text-align: center;">--</div>	1												
A	WO, A1, 8901348 (TEIJIN LIMITED) 23 February 1989, see abstract; figures 5-8 <div style="text-align: center;">-- -----</div>	1												
<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p>* Special categories of cited documents:¹⁰</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="width: 50%;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance, the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance, the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&" document member of the same patent family</p> </div> </div>														
IV. CERTIFICATION <table style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 50%; border: 1px solid black; padding: 5px;"> Date of the Actual Completion of the International Search 29th November 1991 </td> <td style="width: 50%; border: 1px solid black; padding: 5px;"> Date of Mailing of this International Search Report 1991 -12- 9 3 </td> </tr> <tr> <td style="border: 1px solid black; padding: 5px;"> International Searching Authority <div style="text-align: center;">SWEDISH PATENT OFFICE</div> </td> <td style="border: 1px solid black; padding: 5px;"> Signature of Authorized Officer <div style="text-align: center;">  Lena Johansson </div> </td> </tr> </table>			Date of the Actual Completion of the International Search 29th November 1991	Date of Mailing of this International Search Report 1991 -12- 9 3	International Searching Authority <div style="text-align: center;">SWEDISH PATENT OFFICE</div>	Signature of Authorized Officer <div style="text-align: center;">  Lena Johansson </div>								
Date of the Actual Completion of the International Search 29th November 1991	Date of Mailing of this International Search Report 1991 -12- 9 3													
International Searching Authority <div style="text-align: center;">SWEDISH PATENT OFFICE</div>	Signature of Authorized Officer <div style="text-align: center;">  Lena Johansson </div>													

**ANNEX TO THE INTERNATIONAL SEARCH REPORT
ON INTERNATIONAL PATENT APPLICATION NO. PCT/SE 91/00601**

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report. The members are as contained in the Swedish Patent Office EDP file on 31/10/91. The Swedish Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A1- 00404454	90-12-27	JP-A- 3037077	91-02-18
US-A- 4265236	81-05-05	NONE	
WO-A1- 8901348	89-02-23	AU-B- 608895	91-04-18
		EP-A- 0328685	89-08-23
		JP-T- 2500172	90-01-25